

Development of sampling method for cerebrospinal fluid in mice and effect of sampling method on drug concentration in cerebrospinal fluid

Noriyasu Sano, Teruki Hamada,
Shuntarou Tsuchiya, Sayaka Nakagawa
and Nobuyuki Amano

Drug Disposition & Analysis, Research Division, Axcelead Drug Discovery Partners, Inc.



Purpose

Since the sampling of cerebrospinal fluid (CSF) from mice was difficult due to mouse body size, we developed a sampling method and a novel sampling device for the CSF from mice. We investigated the contamination ratio of blood to the CSF due to the sampling method. Furthermore, The effect of the contamination on drug concentration in the CSF was also evaluated by using tool compounds.

Materials and Methods

Development of sampling method for cerebrospinal fluid in mice : Mice and rats were anesthetized by inhalation of isoflurane, and the blood and the CSF were collected from the caudal vena cava and the cisterna magna, respectively. The weight of the collected CSF was measured. The CSF volume was estimated from the weight on the assumption of specific gravity as 1. Red blood cells in the blood and the CSF were counted. The contamination ratio of the CSF by the blood was calculated as the number ratio of red blood cells in the CSF (RBC_{CSF}) to those in the blood (RBC_{blood}).

Effect of blood contamination on drug concentration in CSF (C_{csf}): Metformin, ranitidine, ibuprofen, imipramine, glimepiride, glibenclamide and nefazodone were administered to mice (8W) intraperitoneally. Plasma, brain and CSF samples were obtained after dosing. **CSF was collected deliberately contaminated with blood.**

All animal protocols were approved by the Institutional Animal Care and Use Committee of Shonan Research Center, Takeda Pharmaceutical Company Ltd.

Bioanalysis : Concentrations of metformin, ranitidine, ibuprofen, imipramine, glimepiride, glibenclamide and nefazodone in samples were quantified by LC/MS/MS analysis.

Unbound fraction: Unbound fraction of compounds in plasma and brain was measured by equilibrium dialysis method ($f_{u,p}$ and $f_{u,b}$, respectively)

Results

The novel method of mouse CSF collection




Fig. 1. The collection of CSF from mice.




Fig. 2. Histogram of blood contamination ratio in mouse and rat CSF.

Table 1 Collection amount of mouse CSF and rat CSF

	Amount of CSF (μ L)	
	Mouse	Rat
Mean	11.8	159.2
SD	2.9	26.2

Table 2 Unbound fraction of 7 compounds in mouse plasma and brain

Compounds	$f_{u,p}$	$f_{u,b}$
Metformin	1.0	0.808
Ranitidine	1.0	0.571
Ibuprofen	0.12	0.263
Imipramine	0.10	0.010
Glimepiride	0.030	0.077
Glibenclamide	0.030	0.055
Nefazodone	0.020	0.004

$$\text{Contamination ratio} = \frac{RBC_{CSF}}{RBC_{blood}}$$

Effect of blood contamination on C_{csf}

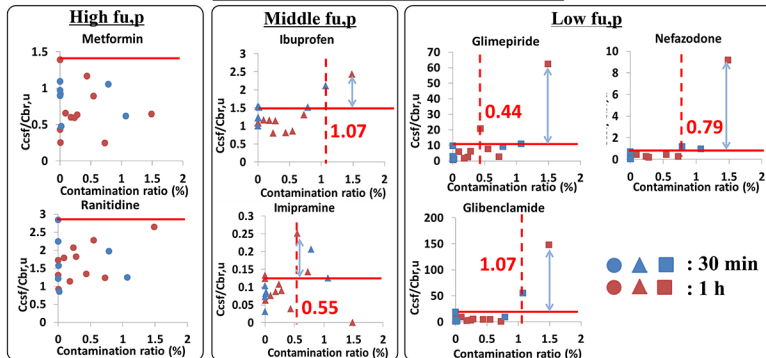


Fig. 3. Relationship of the values $C_{csf}/C_{br,u}$ with contamination ratio (%).

$C_{br,u}$ = Brain conc., $x_{f,u,b}$ = $f_{u,b}$. Red lines indicate maximum $C_{csf}/C_{br,u}$ at which contamination is 0%. Red dotted lines indicate minimum contamination ratio at which $C_{csf}/C_{br,u}$ exceeds red line.

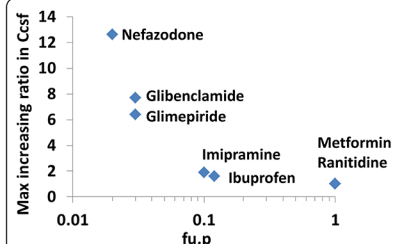


Fig. 4 Correlation between $f_{u,p}$ and increasing ratio by contamination in Csf.

Max increasing ratio in Csf was calculated by the following formula,
Max increasing ratio in Csf = $[C_{csf}/C_{br,u}]_{max}/[C_{csf}/C_{br,u}]_{nc}$.
 $[C_{csf}/C_{br,u}]_{max}$ is maximum value of $C_{csf}/C_{br,u}$.
 $[C_{csf}/C_{br,u}]_{nc}$ is maximum value of $C_{csf}/C_{br,u}$ in samples without contamination.

C_{csf} and $C_{br,u}$ by correction based on contamination ratio

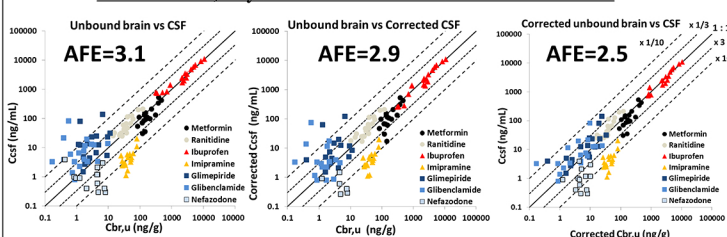


Fig. 5. The correlation between C_{csf} and $C_{br,u}$ by correction based on contamination ratio.

Average-fold error (AFE) = $10^{(1/N \times \sum |Log(Predicted/Actual)|)}$

$$\text{Corrected } C_{csf} = \frac{C_{csf} - \text{Plasma conc.} \times \text{Contamination ratio}}{1 - \text{Contamination ratio}} \quad \text{Corrected } C_{br,u} = \frac{C_{br,u} + \text{Plasma conc.} \times \text{Contamination ratio}}{1 + \text{Contamination ratio}}$$

Summary

- ✓ We established a method of CSF sampling from mice with maximum contamination ratio of 0.14%
- ✓ Minimum contamination ratio which affected compound concentration in CSF was 0.44%.
- ✓ The compounds with lower $f_{u,p}$ tended to show the larger effect on concentration ratio.
- ✓ AFE value between C_{csf} and $C_{br,u}$ was improved by correction based on contamination ratio.

Conclusion

We established a method of CSF sampling from mice applicable to the evaluation of compound concentration in CSF.

COI disclosure information

We have no financial relationship to disclose for our presentation contents.